BR58 Body Shape Skin Beauty System

3D **Breakthrough Technology for body reshaping**

USER MANUAL

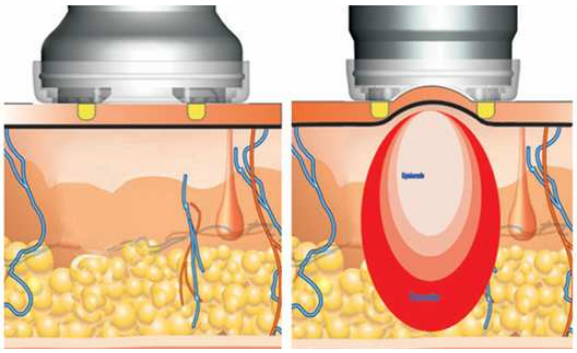

Theory Pictures

Honorable Clients

Thanks for your attention to our products BR58 Body Shape Skin Beauty System .
For better use this machine,please read through the user manual and follow the isntruction of this machine in detail when you operate the machine.

It forbids someone to open and remove the mainframe of this machine besides authorized from the our company.

Please contanct our in time if there are any question during operation.

Professional technique from our company to satisfy your kinds of requirements in a good way.

Theory Instruction

Radio Frequency (RF)

The release of high-frequency 1MHZ polynomial radiofrequency, energy is mainly used to shuttle between the focus on the multi-polar, then the required response to treatment, combined with the simultaneous release of negative pressure, so that 100% of the treated area can be completely absorbed RF energy to achieve the transformation of the dermis . High frequency makes the body heat, when the dermal tissue to reach 46 degrees heat, which produces the contraction of collagen fibers and stimulate the secretion of new collagen to fill more atrophy and loss of collagen, gap, with the continued proliferation of dermal collagen and re- arrangement, allowing relaxation of the skin in the course of treatment, immediately feel the upward, compaction of the lift effect. Bracket to show the soft skin, when a growing number of collagen, the dermis layer of skin thickness and density increase, fill wrinkles, remove scars, skin elasticity and re-gloss gray, white skin look fresh, be calm wrinkles, sagging The skin becomes full, compact, and flexible.

Vacuum

Vaccum or Negative pressure through specially designed suction head, which with the function of skin beauty and muscle massage, will improve the flow of body fluids between cells, thereby increasing the movement of cells, activation of cells to improve skin elasticity, and fine blood vessels can accelerate blood circulation, and the body excess to drain away toxins, reduce facial spots and pigment and other adverse factors, the probability of the formation, and improve edema and other issues.

Vaccum function with more adjustment six different modes for different treatment according to different kinds of need to make continuous or intermittent negative pressure of the pulse output, offering the most personal and comfort care.

Physical, the ground-breaking treatment of head shape designed to allow more manipulation beautician handy. At the same time, it will be efficient bipolar radio frequency, to bracket the bottom of the distribution in the treatment of head, with simultaneous output of negative pressure to ensure that radio frequency energy hundred percent direct to deep fat layer, to achieve the best fat burning results.

CAVITATION (35KHZ Ultrasonic)

Ultrasound slimming technology is coupled by way of contact with the body no harm frequency and power which with low frequency ultrasonic energy transfer to different parts of the adipose tissue to the use of ultrasonic cavitation principle. For adverse pathological adipose tissue, using the energy generated by cavitation so that fat cells rupture. After rupture of fat cells and body fluids circulating phagocytic macrophages, will reduce the number of fat cells, reach slimming weight loss goals.

FUNCTION

1. Radio Frequency

A. what is the RF ?
The use of radio frequency electromagnetic fields generated by the concept of the development of energy compatible with the human body, so that high-frequency current caused by electromagnetic fields produced through bio-thermal effect, the movement of ions to drive the body to produce heat to reach the effect of dissolving fat.

Remarks: the concept of induction cooker, oven with a metal ring, when the current through the coil, the magnetic field, changing the magnetic field, collisions, rotation, distortion, resulting in thermal energy (bio-energy) which need to be liquid medium.

Security: Current will not stimulate the sensory nerves and motor nerves.

So: 1.Does not cause muscle contraction.
2. When electrons move inside the body which generates heat.

B. RF stimulus:
An innovative technology, the movement of molecules caused by the 5-15mm deep tissue to produce heat, so the depth of adipose tissue to heat up, increasing the oxygen within the cell, thereby stimulating the deep micro-circulation, production of collagen, increase cell penetration .

C. The specific effect:
A. Through bio-energy, increase the temperature of the deep, deep fat body completely break.
B. Improve lymphatic circulation, accelerate fat burning,
C. Speed up metabolism, increase body fat accumulation ability of spontaneous combustion.
D. Drain away toxins and waste, healthy fiber

2. Negative Pressure

A. Negative pressure was first used in the medical school, regular exercise can not give some of the current operation can be used in human populations, to help with physical therapy, passive exercise, and found to effectively prevent muscle atrophy, muscle and fat ratio close to normal. A lot of medical proof that a negative pressure on the lymphatic circulation of the force, the depth of scientific research have taken different amount of pressure, making treatment more accurate.

B. Negative pressure effect:
Negative pressure is a humanoid hand massage to help break down fat fat movement, using a dedicated manufacturing operation of the first negative pressure, the skin on the regularity of negative pressure massage to hard fat, fiber breakage, and promote lymphatic drainage, drainage and increase skin elasticity effect.

C. Treatment effect:
(1).Remove excess fibers from tissue water.

(2) And strengthen blood vessels and improve varicose veins.
(3) To break the cellulite hard fiber, making it more flexible and to shaping the results.

D. Comparison with similar instruments
(1) Roller LPG (M6) hand tool handle heavy, can only walk straight lines can not meet the characteristics of people, pick up the skin to be strong, easy bleeding, power consumption, while not using the product because the wear coat.
(2). CFK ball style, Xichuo too little space, to reduce the effects of liposuction, not with products, cleaning difficult.

Features

1. Normally, Commen radio-frequency heat treatment can reach 3-15mm depth, which also need take 15-20 minutes to reach the temperature of break down fat . The bipolar radiofrequency only need 2 minutes.

2. Intelligent design curve for the operation of the human head for more efficient, more effective in preventing head Olive liposuction fat pinched in the process of fat loss, reduce pain, enhance the effect of dissolving fat.

NOTES

1. Taboo crowd

1). Pregnant or lactating women
2). Epilepsy, cancer, acute inflammation and wound infection, surgical wound healing in patients not
3). Heart disease or with heart pacemakers, kidney disease (cholelithiasis), severe diabetes
4). Heart, brain, nerve center of the neck, spine, eye, bleeding, injection, metal parts of the uterus Global (to treat other parts of the)
5). Menstruation, birth control period or period of urinary incontinence, abdominal surgery, who did
6). With atopy, severe telangiectasia, prolonged use of steroids may and endocrine disorders (treat other parts of the)
7.) Hemophilia or severe bleeding
8.) High fever, body heat, there are a lot of people.
9. Psoriasis, hyperthyroidism, skin cancer, asthma, hypertension, congenital immune deficiency.

2. Operation notes

1) Check the power cable before turning on power, must be shut down when not in use, first power off the fuselage, and then pull the power cord.
2) The operator and the user must remove the metal parts, do not use the telephone and avoid all interference with communications products.
3) When you need specialized equipment in the high-frequency cream, body cream because there is such ions with other products easy to produce sparks.
4) Do not suddenly change the pressure or too much RF energy
5) the beginning of each treatment more than asking guests feel at any time to adjust the parameters
6) For detoxification row edema, the pressure and RF energy value should be reduced.
7) The hard, thick parts: RF1MHZ, pressure 0.09MPA or more (depending on the affordability of the guests); actions: pull up about to go look, shake-style walking, so that the organization loose, soft.
8) The same day can not use current equipment, such as in vivo plasma to be dispersed.
9) Note communicate with customers during the operation temperature, as guests are able to withstand heat, are easy to cause damage.
10) a course of time, not at the same time to accept other treatments.

3. Equipment maintenance and cleaning

1).daily body rub with a dry towel,
2).operating under the head after use screw caps, water-soaked with alcohol dry clean cotton, the first operation must be kept clean and avoid scratching the surface.
3). to prevent direct sunlight to prevent vibration and swinging equipment and instruments
4). the treatment can not be too high when the indoor temperature
5). regular inspection of aircraft after the external filter is clean and timely replacement.
6).continued use of the instrument too long (about 1-1.5 hours), will need to shut down rest for 10-15 minutes.
7). the instrument off when not in the body first and then disconnect the power supply, lock the bottom pulley apparatus.

Operation Instruction

Enter Operate Screen after turn on machine

Set for Handle pieces

Big Handle piece screen

RF Intensity

Six different rhythem modes

Vaccum Instensity

Time Set

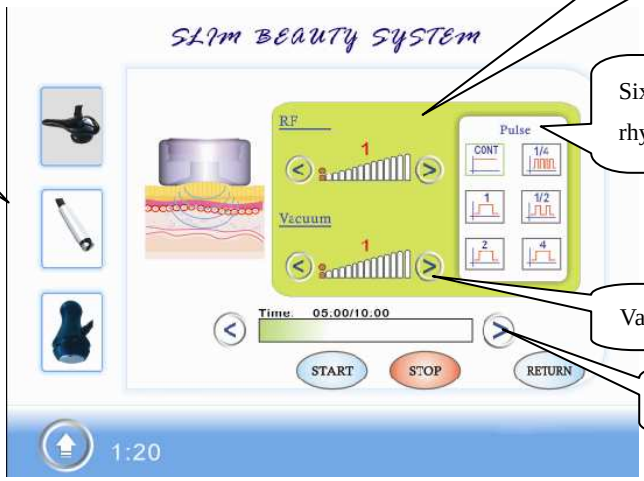

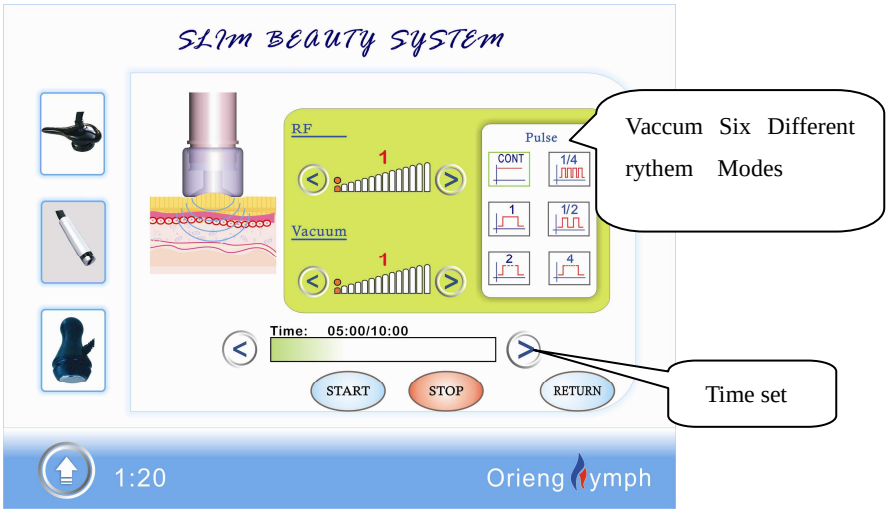

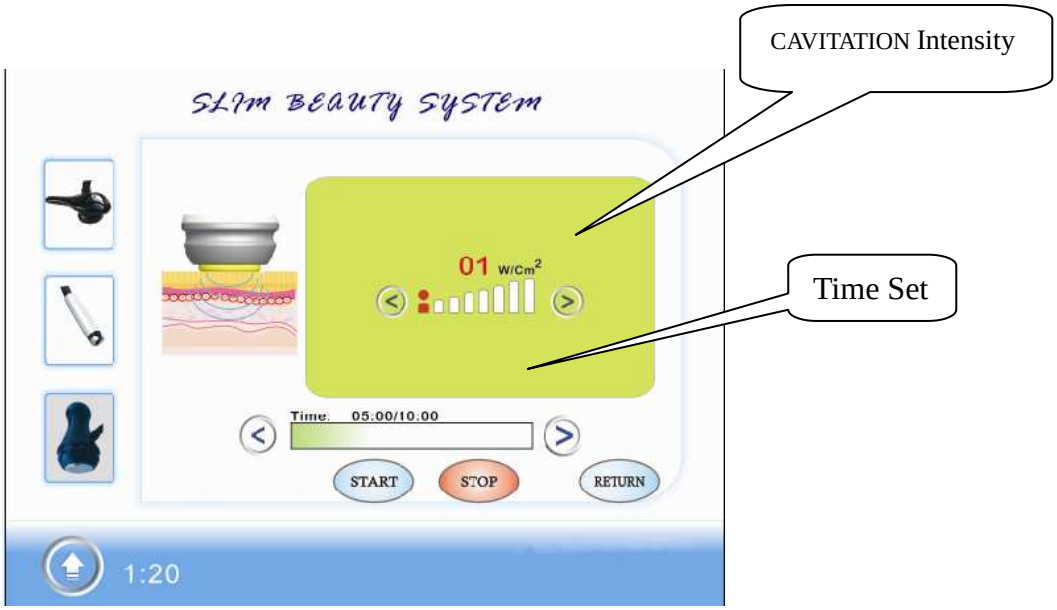

Threatment plan

1. Lose weight: 2-3 times per week, 20-30 times for one course, minus 3-7CM; 30-35 minutes per site;

Effects: qualitative wrinkles (70% -80% improvement) to be treated 12 times

Pseudo-wrinkle: one treatment (70-80% improvement)

Fine lines: one to eliminate

Note: Depending on individual circumstances, do it for 1-2 courses, the effect is sustainable for 3-6 months.

ATTENTION NOTES

An instrument can not eat two hours before and after;
2 instrument used to drink a glass of water before, after drinking at least eight glasses of water;
3 instrument use you removed the body to wear metal objects and mobile phones;
4 treatment, the treatment area must be applied gel operation;
5 vacuum suction head operation, should be based on reasonable changes in the frequency of operation;
6 treatment head must be close to the skin, can not operate at the same site overlay;
7 hypertension, cancer, diabetes, heart disease, skin disease, severe varicose veins and skin allergy patients is prohibited during the operation;
8 should not operate waist and abdomen during menstruation, postpartum, as the case do (natural delivery after three months, six months after Caesarean section)
9 recommends that customers:
First, regular exercise, to accelerate fat burning, muscle strengthening, and activation of lower limb blood circulation;
Second, develop good eating habits, such as a balanced diet, eat more foods rich in minerals and vitamins, regular meals, avoid snacking and prolonged fasting;
Third, there are regular daily drinking enough water

Technical parameters

1. The host size: 48CMX49CMX118CM (144CM with frame)
2. The Outside package: 56CM x 66CM x 138CM
3. The use of power: 220V/50Hz or 110V/60Hz
4. Display: 8 inch color touch screen
5. Power Consumption : ≤400W
6. Regular time: 60 minutes
7. The fuse size: F3AL250V
8. RF Frequency: 1MHz
9. Cavitation with frequency: 35KHz
10. Vaccum Pressure: 100Kpa
11. LED Wave Length:Red: 635nm Green: 525nm Blue: 470nm
12. N.W: 40KGS; G.W: 60KGS